

# Agilent U1241B and U1242B **Handheld Digital Multimeter**

### **Ouick Start Guide**





The following items are included with your multimeter:

- Silicone test leads and 4mm probes




- Printed Quick Start Guide
- Four 1.5 V AAA alkaline batteries
- Certificate of Calibration

If anything is missing or damaged, please contact the nearest Agilent Sales Office.


For more detailed information, please refer to the Agilent U1241B and U1242B Handheld Digital Multimeter User's and Service Guide on Agilent Web site (www.agilent.com/find/handheld-tools).

WARNING Ensure the terminal connections are correct for that particular measurement selection before starting any measurement. To avoid damage to the device, do not exceed the input limit.

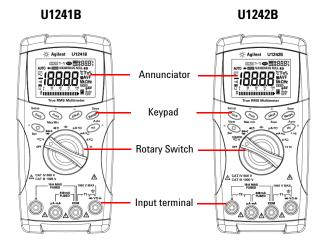

Measurement Functions	Input Terminal		Overload Protection
Voltage			1000 V R.M.S
Diode	→LVΩ-J-L	СОМ	1000 V R.M.S < 0.3 A short circuit current
Resistance	P1 V12 /1		
Capacitance			ourront.
Current (µA and mA)	μA.mA	СОМ	440 mA/1000 V 30 kA/fast-acting fuse
Current (A)	А	СОМ	11 A/1000 V 30 kA/fast-acting fuse
Temperature	+T1	-T1	1000 V R.M.S
Temperature (for U1242B)	+T2	-T2	440 mA/1000 V 30 kA/fast-acting fuse

# **Annunciator Display**

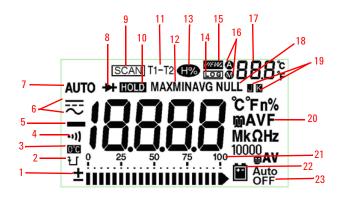


No.	Descriptions	No.	Descriptions
1	21-segment analog bar graph display	12	MINMAX Recording mode
2	Capacitor discharge indicator	13	Harmonic Ratio mode (for U1242B)
3	Cold junction of ambient temperature	14	Data logging mode (for U1242B)
4	Audible continuity for resistance and diode function	15	Data logging viewing mode (for U1242B)
5	Primary display -1888	16	Auto or manual data logging mode and datalog viewing mode
6	AC or DC measurement mode	17	Secondary display (temperature display)
7	Auto range	18	Null math function
8	Diode / Audible continuity	19	Thermocouple type for temperature measurement
9	T1, T2 and T1 – T2 temperature	20	Primary measurement units
	measurements scan (for U1242B)	21	Measurement range
10	Data hold	22	Low battery indicator
11	T1, T2* and T1 – T2* temperature measurements	23	Auto power off indicator

<sup>\*</sup>T2 temperature measurement and delta (T1 - T2) are only available for U1242B.

## **Functions and Features**

## **Rotary Switch**

## Keypad









Scan	
	0

Function	First level functions	Range	Second level functions (press Shift )	Range
OFF	Turn off the meter			
H.RATIO V	DCV measurement	0.1 mV to 1000 V	ACV measurement	0.1 mV to 1000 V
			Harmonic ratio (for U1242B)	0.0% to 99.9%
SW-C	Diode measurement		Switch counter measurement	
<b>4</b> 1)) Ω	Resistance measurement	0.1 $\Omega$ to 100 M $\Omega$	Audible continuity measurement	
<b>→</b> ⊢	Capacitance measurement	0.1 nF to 10 mF		
μА≂	DCμA	0.1 μA to 10 mA	ACμA measurement	0.1 μA to 10 mA
mA≂	DCmA	0.01 mA to 440 mA	ACmA measurement	0.01 mA to 440 mA
			mA% scale	
A≂	DCA	0.001 A to 10 A	ACA measurement	0.001 A to 10 A
T1	T1 temperature	-40°C to 1000°C	T2 and T1–T2 temperature measurements (for U1242B)	-40 °C to 1000 °C

Action	Steps
Turns ON backlight	Press 🔅 .
Checks battery capacity	Press and hold of for >1 s.
Freezes the measured value	Press Hold .
Starts MIN/MAX/AVG recording	Press and hold Hold for >1 s.
Offsets the measured value	Press (aNull).
Scan the measured temperature (for U1242B only)	Press and hold (ANull) for > 1 s.
Changes the measuring range	Press (Range).
Turns on auto range	Press and hold Range for > 1 s.
Measures frequency for AC signal	Press Hz.
Starts manual data logging	Press and hold Hz for > 1 s.

#### **Tilt Stand**



Tilt stand at 60 °



Tilt stand at 30 °

#### **Safety Notices**

CAUTION

A CAUTION notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in damage to the product or loss of important data. Do not proceed beyond a CAUTION notice until the indicated conditions are fully understood and met.

#### WARNING

A WARNING notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in personal injury or death. Do not proceed beyond a WARNING notice until the indicated conditions are fully understood and met.

### **Safety Information**

The Agilent U1241B and U1242B are safety-certified in compliance with the following safety and EMC requirements

- following safety and EMC requirements:
  IEC 61010-1:2001 / EN61010-1:2001
- USA: UL 61010-1:2004
- Canada: CSA C22.2 No. 61010-1:2004
- IEC 61326-1:2005/ EN 61326-1:2006
- Canada: ICES/NMB-001:2004
   Australia/New Zealand: AS/NZS CISPR11:2004

#### **Safety Symbols**

=	Earth (ground) terminal
	Equipment protected throughout by double insulation or reinforced insulation
A	Caution, risk of electric shock
$\triangle$	Caution, risk of danger (refer to the instrument manual for specific Warning or Caution information)
CAT III 1000 V	Category III 1000 V overvoltage protection
CAT IV 600 V	Category IV 600 V overvoltage protection

For further safety information details, refer to the Agilent U1241B and U1242B Handheld Digital Multimeter User's and Service Guide.

Second Edition, June 14, 2012 © Agilent Technologies, Inc., 2009–2012

