


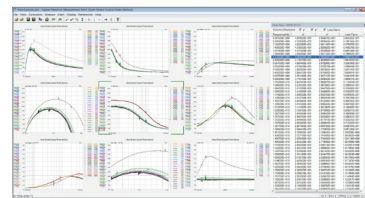
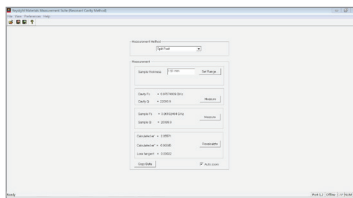


Keysight Technologies N1500A Materials Measurement Suite

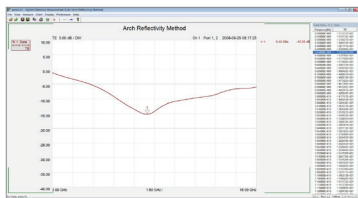

Technical Overview

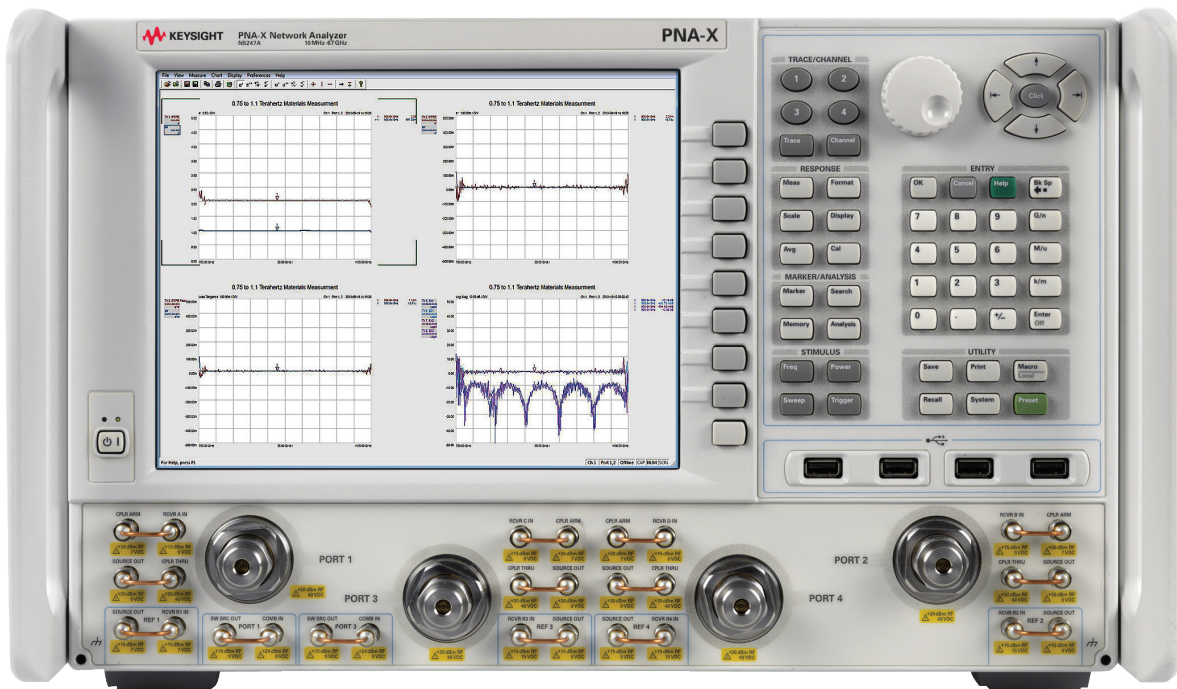

Features

- Software automates complex permittivity and permeability measurements
- Flexible option configuration allows you to choose the measurement methods you need
- One simple installation program and integrated method option loader switches seamlessly between the different measurement methods:



- Transmission line and free space



- Arch reflectivity



- Resonant cavity



- Coaxial probe

- Runs on Windows XP, Windows 7 and Windows 8
- Download a free trail from our web site: <http://na.support.keysight.com/materials/downloads.html>

Automate complex permittivity and permeability measurements with Keysight's materials measurement software suite

Measure ϵ_r^* and μ_r^* over a wide frequency range

With Keysight N1500A materials measurement software suite, you can determine the intrinsic electromagnetic properties of many dielectric and magnetic materials. The complete system is based on a versatile Keysight network analyzer which measures the material's response to RF or microwave energy. The N1500A software controls the network analyzer and calculates results. Depending on the Keysight network analyzer and sample holder used, frequencies can extend from the mid-MHz to the low THz.

Powerful features

- Multiple channel and port selections provide maximum flexibility when setting up network analyzers with up to four ports.
- Multiple charts and traces aid in data analysis. Depending on method option selected, data can be displayed in a variety of formats:
 - Permittivity: ϵ_r , ϵ_r' , $\tan \delta$, Cole Cole
 - Permeability: μ_r , μ_r' , $\tan \delta_\mu$
 - S-parameters: log mag, linear mag, phase, unwrapped phase, group delay, smith chart, polar chart, real, imaginary, and SWR
 - Trace math functions: +, -, *, /, mean and standard deviation
 - Trace data pane: displays the active data trace in tabular format

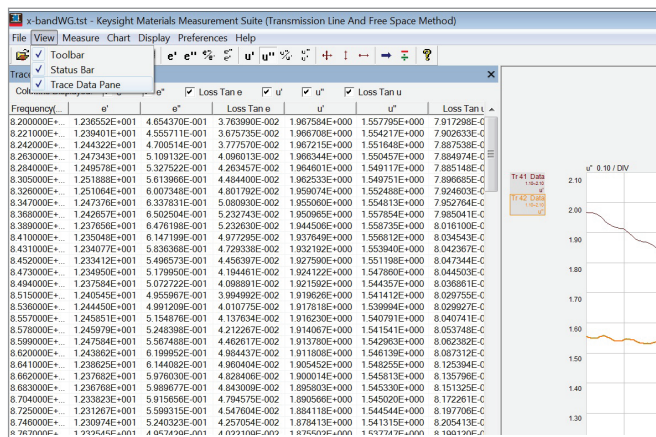


Figure 1. Configurable trace data pane allows you to choose if and where it is displayed and which data columns to include.

- Markers with reference and delta functions and rubberband zoom scaling allow close inspection of critical data.
- Off line mode allows software to run on a PC without being connected to an instrument. Free up shared network analyzer resources by taking your data analysis back to your desk, or wherever you want!
- S-parameter import and save
- Measurement report captures trace and tabular data, equipment used, sample description, user name, date and more in a professionally formatted document ready to print, save, or send electronically in an Adobe Acrobat (.pdf) file.

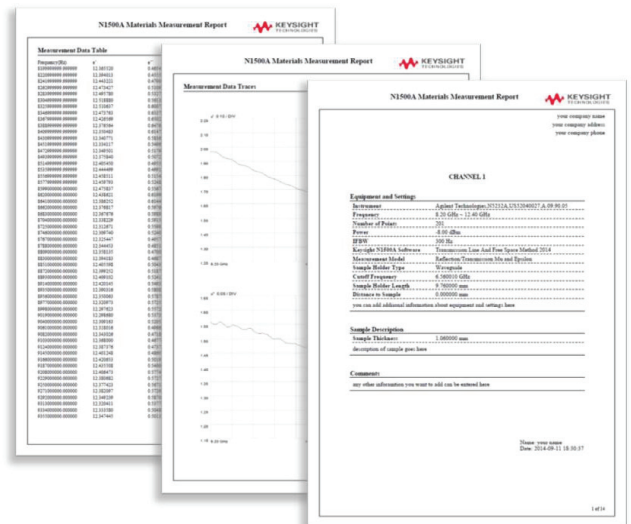


Figure 2. Measurement reports

Connect to other programs

Data can also be saved in a variety of formats to bring into other programs for reporting or further data analysis. An application programmable interface (API) allows the measurements to be set up, triggered and read from a user written program.


Software Update Service (SUS)

Materials measurement suite has an annual update called “SUS” that stands for “Software Update Service”. Each new license comes with 12 months of SUS. After 12 months, a 1 year extension can be purchased to allow continued software updates and technical support.

Measurement method options

Keysight offers a variety of measurement methods to meet the needs of most materials under test. Each method has its own strengths and limitations that make it more or less useful for a particular application. Flexible option configuration allows you to choose one or more methods to meet your specific needs.

Transmission line and free space method – Option 001



The sample is placed in a guided transmission line such as a coaxial airline or waveguide straight section, or suspended in free space between two antennae. Several algorithms to calculate permittivity and permeability from S-parameter measurements are available to choose from.

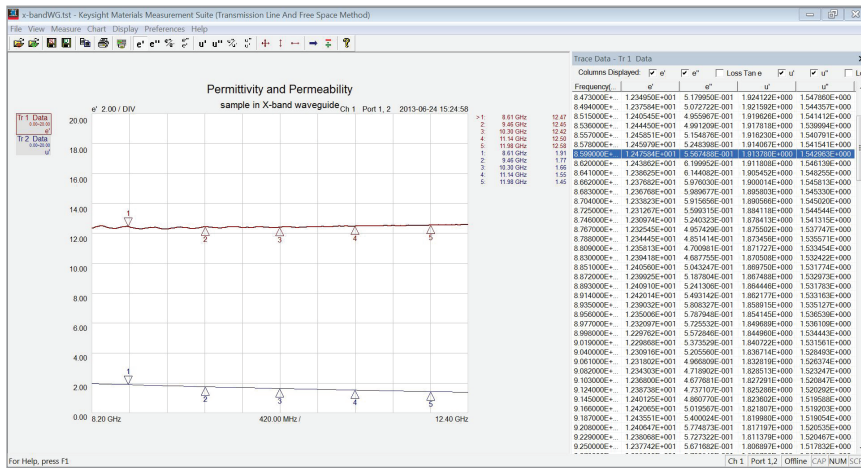


Figure 3. Example of transmission line measurement results.

Transmission Line

Coaxial airlines or rectangular waveguide transmission lines are used as sample holders. The transmission line method works best for materials that can be precisely machined to fit inside the sample holder. The N1500A Option 001 includes an algorithm that corrects for the effects of air gap between the sample and holder, reducing the largest source of error with the transmission line technique.

Typical transmission line system configuration

- *Keysight network analyzer*
- Waveguide or coaxial transmission line for sample holder
- Waveguide or coaxial calibration kit to match sample holder connectors
- A pair of test port cables
- Adapters as required to connect cables to network analyzer and sample holder

Free space

In this method, materials are placed between two antennae for a non-contacting measurement. The free space method works best for large flat solid materials, but granular and powdered materials can also be measured in a fixture. It is very useful for many applications such as non-destructive testing, measuring materials that must be heated to very high temperatures, or measuring a large area of material that is non-uniform such as honeycomb or a composite.

Typical free space system configuration

- *Keysight network analyzers*
- Free space fixture consisting of a pair of horn antennae, sample holder and metal plate for calibration. Antenna should be placed approximately $2d^2/\lambda$ from the sample, where d is the larger antenna aperture dimension.
- Waveguide or coaxial calibration kit to match horn antennae input connector
- A pair of test port cables to reach from network analyzer ports to free space fixture (not required for millimeter-wave systems where horns are usually connected to millimeter-wave frequency extender modules).
- Adapters as required to connect cables to network analyzer and sample holder

Powerful free space calibration and gating techniques

Gated isolation/ response calibration reduces errors from diffraction effects at the sample edges, and multiple residual reflections between the antennas. Gated reflect line (GRL) calibration makes accurately calibrating in free space fast and easy. A software wizard automatically sets up all the free space calibration definitions and network analyzer parameters, saving engineering time. It reduces costs associated with TRM and TRL calibration methods by eliminating the need for micro antennae positioners or direct receiver access.

There are now two ways to perform GRL calibration. The original 2 tier GRL calibration technique converts a previously saved full 2-port coaxial or waveguide calibration into a full 2-port free space calibration by measuring two additional standards, the empty free space fixture and a metal plate. With 1 tier GRL cal, a waveguide or coaxial cal is not required before the metal plate and empty fixture measurements. Because 1 tier GRL cal requires a longer alias free time domain span, it is best suited for set ups that don't have long cables, when the frequency span is not extremely wide, or a large number of points is not desired. GRL calibration requires a network analyzer with full S-parameter (S11, S21, S12, S22) capability and time domain option. An appropriate free space fixture with metal calibration plate is also needed.

Mathematical models

Option 001 has nine different algorithms to choose from, each with benefits for different materials and applications. The reflection transmission model described by Nicolson and Ross, is best for magnetic materials such as ferrites and absorbers. It calculates both ϵ_r^* and μ_r^* (including loss) from a two-port measurement of a single sample. There are two additional two-port algorithms for non-magnetic materials ($\mu_r^*=1$). These models do not suffer from discontinuities at frequencies where the sample length is a multiple of half-wavelengths like the Nicholson Ross model and are best for long, low-loss materials. The two polynomial fit models can smooth out the effects of measurement error due to noise and mismatch, but are not suitable for materials that have sharp narrow band responses.

While the two-port algorithms are best for most solid materials, one-port algorithms provide a simple calibration and measurement, and can be better suited to measurements of liquids and powders. For example, a shorted waveguide can be turned on end vertically and filled with a material for a one-port measurement. One-port fixtures are also better suited for high-temperature measurements where one end of the fixture can be heated, while cooling mechanisms at the other end protect the network analyzer. Although one-port fixtures are usually terminated with a short circuit, the N1500A-001 also accommodates an arbitrary termination which produces more reliable results for thin samples.

N1500A	Alternate	S-parameters measured	Result	Description	References
Reflection / Transmission Mu and Epsilon	Nicholson-Ross-Weir, NRW	S11, S21, S12, S22	ϵ_r, μ_r	Originally developed by Nicholson and Ross, and later adapted to automatic network analyzers by Weir to calculate permittivity and permeability from transmission and reflection coefficients. Can have discontinuities for low loss samples with thickness of $> \frac{1}{2}$ wavelength. Best for magnetic materials such as ferrites and absorbers.	AM. Nicolson and G. F. Ross, "Measurement of the intrinsic properties of materials by time domain techniques," IEEE Trans. Instrum. Meas., IM-19(4), pp. 377-382, 1970. W.W. Weir, "Automatic measurement of complex dielectric constant and permeability at microwave frequencies," <i>Proc. IEEE</i> vol. 62 pp.33-36, Jan 1974
Reflection / Transmission Epsilon Precision	NIST Precision	S11, S21, S22	ϵ_r	Developed by NIST to calculate permittivity from transmission and reflection coefficients. Best for longer samples of low-loss dielectric materials.	Improved Technique for Determining Complex Permittivity with the Transmission/Reflection Method, James Baker-Jarvis et al, IEEE transactions on microwave Theory and Techniques vol 38, No. 8 August 1990.
Transmission Epsilon Fast	Fast Transmission	S21, S12	ϵ_r	An iterative technique that estimates permittivity and then minimizes the difference between the S-parameter value calculated from that permittivity and the measured values until the error is less than the expected system performance. Uses only transmission parameters S21, S12, or the average of S21 and S12. Best for longer samples of low-loss dielectric materials or for systems with significant reflection error.	Not Published

N1500A	Alternate	S-parameters measured	Result	Description	References
Polynomial Fit Reflection / Transmission Mu and Epsilon	Poly Fit, Bartley	S11, S21, S12, S22	ϵ_r, μ_r	Uses an iterative technique to fit measured S-parameters to a polynomial, incrementing the order of the polynomial until the error is less than the expected system performance. Best for magnetic samples. Not recommended for meta or left handed materials.	P. G. Bartley, and S. B. Begley, "A New Technique for the Determination of the Complex Permittivity and Permeability of Materials Proc. <i>IEEE Instrument Meas. Technol. Conf.</i> , pp. 54-57, 2010.
Polynomial Fit Transmission Epsilon	Poly Fit, Bartley	S21, S12	ϵ_r	Uses an iterative technique to fit measured S-parameters to a polynomial, incrementing the order of the polynomial until the error is less than the expected system performance. Best for magnetic samples. Not recommended for meta or left handed materials.	P. G. Bartley, and S. B. Begley, "A New Technique for the Determination of the Complex Permittivity and Permeability of Materials Proc. <i>IEEE Instrument Meas. Technol. Conf.</i> , pp. 54-57, 2010.
Stack Transmission Mu and Epsilon	Stack Two Transmission	S21, S12 (2 samples)	ϵ_r, μ_r	An iterative technique that uses two transmission measurements. One measurement is of the sample which optionally may be backed by a known dielectric. The second is of the sample, backing and another known dielectric. The model is useful for free space measurements. It requires a full 2-port or a two-port transmission resp/isol cal.	Not Published
Reflection Only Epsilon Short-Backed	Short Backed	S11	ϵ_r	An iterative technique that minimizes the difference between the measured and calculated reflection coefficient of a material backed by a short. The idea of measuring a material backed by a short was published by Von Hippel. Although, Von Hippel uses tables to determine the value of permittivity instead of iteration.	A. R. Von Hippel, Ed. <i>Dielectric Materials and Applications</i> , John Wiley and Sons, New York, 1954)
Reflection Only Epsilon Arbitrary- Backed	Arbitrary Backed	S11	ϵ_r	An iterative technique that minimizes the difference between the measured and calculated reflection coefficient of a material backed by a separately measured backing. This model is an extension of method proposed by Von Hippel. It is useful when the material is electrically short such that the voltage across the material is effectively zero when backed by a short.	A. R. Von Hippel, Ed. <i>Dielectric Materials and Applications</i> , John Wiley and Sons, New York, 1954)
Reflection Only Mu and Epsilon Single/Double Thickness	Single/Double Thickness	S11 (2 samples)	ϵ_r, μ_r	Uses two reflection coefficient measurements to calculate S11 and S21 of the material. The measurements are a sample and a sample that is twice the length as the original. After doing so the Nicolson Ross model is used to determine the material properties.	Not Published

Sample thickness calculator

This utility provides you with a suggested thickness for your sample, given an estimate of the sample's electromagnetic properties and measurement frequency range. Electrical lengths of $\frac{1}{4}$ and $\frac{1}{2}$ wavelength are graphed over frequency so you can optimize for different models. Markers can be added to target specific frequencies of interest.

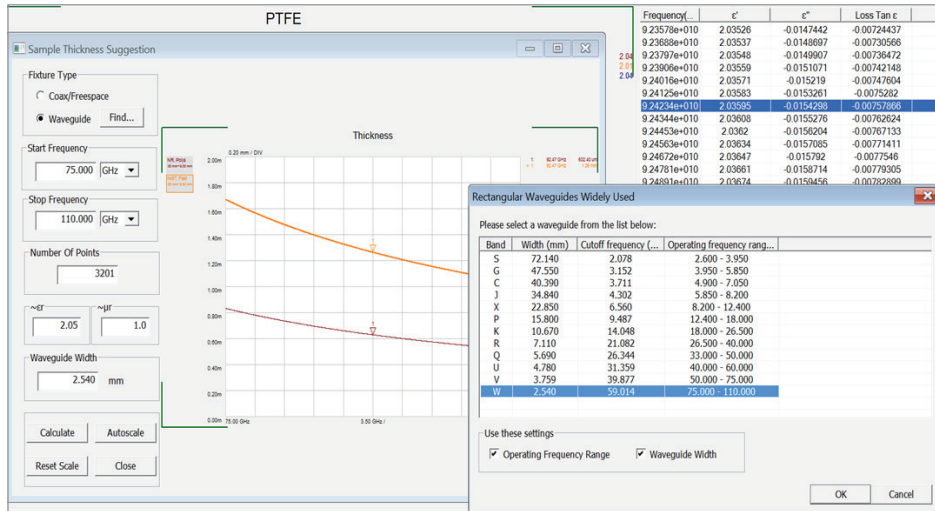


Figure 4. Sample thickness calculator

Discontinuity detector

When measuring low loss samples with a thickness of more than $\frac{1}{2}$ wavelength using the Nicholson Ross Weir model, discontinuities can appear in the trace. The discontinuity detector calculates where this will occur and highlights that portion of trace, giving you the information you need to determine whether or not a response is a true response of your material.

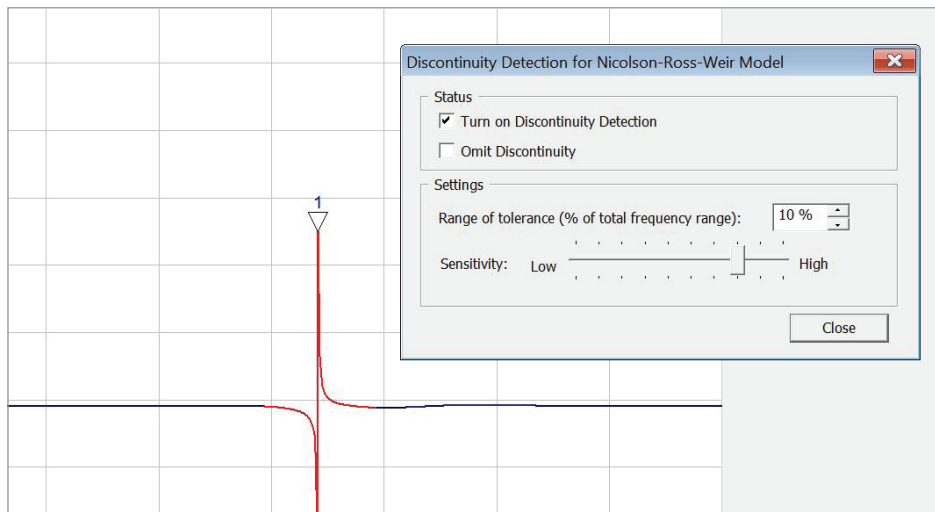


Figure 5. Sample thickness calculator

De-embedding

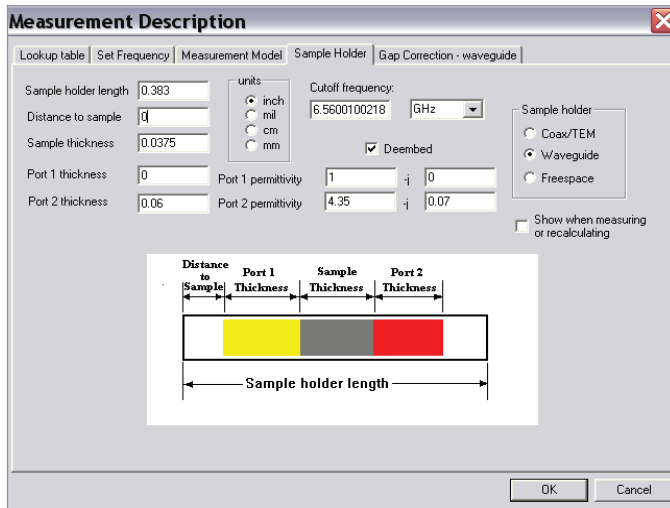


Figure 6. Sample holder definition screen with de-embedding

De-embedding allows a sample to be backed with a dielectric backing on one or both sides. It mathematically removes the effects of the backing, so the electromagnetic properties of just the sample are reported. This is useful when a sample is not stiff or thick enough to stand up by itself, or it cannot be removed from a substrate. The backing must have a known permittivity and thickness. If the permittivity of the backing is not known, it can be measured separately first. The backing material cannot be magnetic and it must allow the microwave signal to transmit through it so that S21 and S12 can be measured.

De-embedding feature works with the following transmission models:

- Reflection/Transmission Mu and Epsilon
- Transmission Epsilon Fast
- Polynomial Fit


Typical frequency range	100 MHz ¹ to 1.1 THz
Material properties	Dielectric and magnetic Material under test is assumed to be homogeneous (uniform composition) with no layers ² Anisotropic materials can be measured in waveguide
Sample form	Most often used for solid materials Sample is assumed to have flat parallel sides
Typical accuracy	1 to 2%
Data formats	Permittivity: ϵ_r , ϵ_r' , $\tan \delta$, Cole Cole Permeability: μ_r , μ_r' , $\tan \delta_\mu$ S-parameters: log mag, linear mag, phase, unwrapped phase, group delay, smith chart, polar chart, real, imaginary, and SWR Trace math functions: +, -, *, /, mean and standard deviation Data pane: view displays trace data in tabular format
File formats	Data and Setup: .tst Data: .prn, .csv Measurement report: .pdf S-parameters: .s2p, .ts
Sample holders and fixtures	For a list of recommended sample holders and fixtures, please see; http://na.support.keysight.com/materials/docs/SampleHolders.pdf

1. Minimum frequency is set by the maximum practical sample length (L): f (in GHz) >

$$\frac{1}{\sqrt{\epsilon_r' \mu_r'}} > \frac{30 \text{ cm}}{L(\text{in cm})} > \frac{20}{360}$$

2. If the material is not homogeneous through the length of the sample (i.e., layers), the reflection from the front (S11) and back (S22) face will be different and will lead to a potentially erroneous result. If the material is not homogeneous across the face of the sample, the result is an average value over the cross section that is exposed to the EM field (weighted by the intensity).

Arch reflectivity method – Option 002



First developed by the U.S. Naval Research Lab, the NRL arch measurement method is a useful technique to test angular dependent absorptive characteristics of a material. The typical setup involves a network analyzer connected to two horn antennas fixed to an arch armature above (or below) a flat piece of the material under test. One antenna operates as the transmitting antenna while the second one receives the reflected signal to complete a one-port measurement. Sample should be in “far field”.

Typical arch reflectivity system configuration

- Keysight network analyzer
- NRL arch fixture
- Cables and adapters as needed

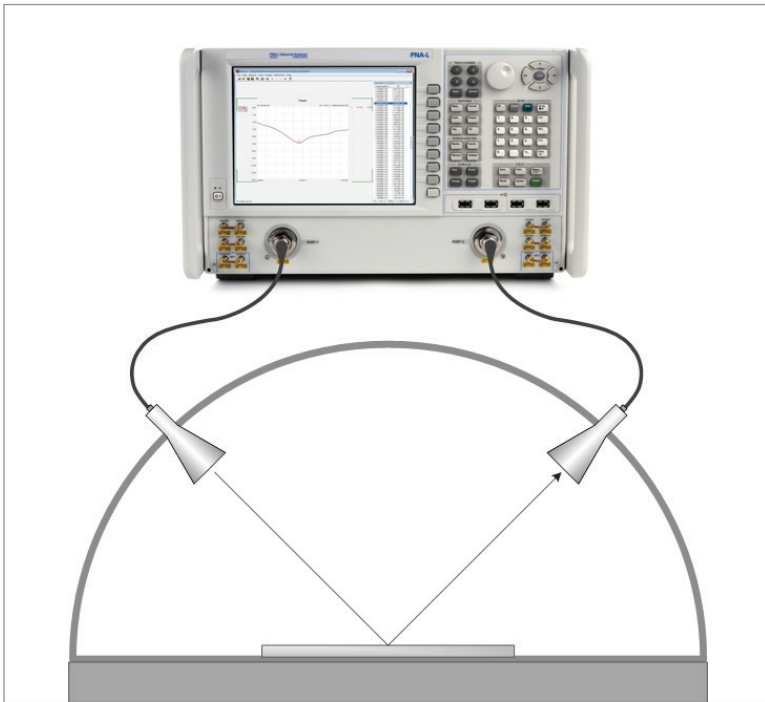


Figure 7. In the NRL arch method, one antenna transmits energy onto the MUT and the second antenna receives the reflected portion.

Option 002 automates NRL arch measurements. The program guides you through the complete process of setup, calibration and measurement of material reflectivity.


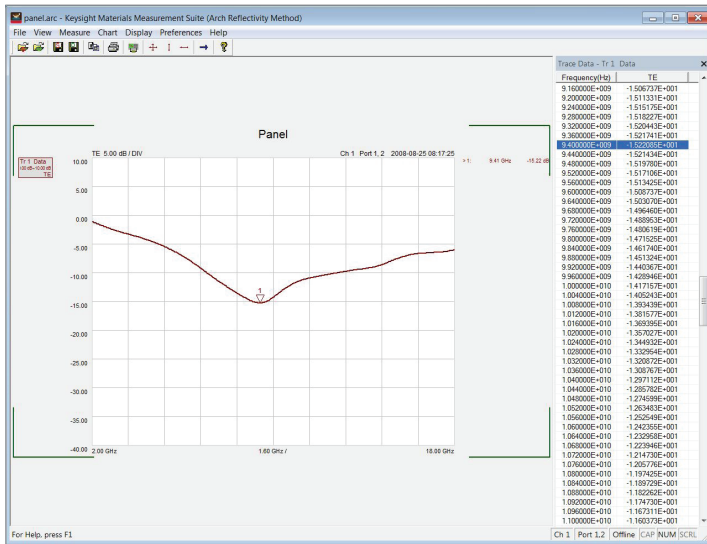


Figure 8. Example of arch reflectivity measurement results.

Typical frequency range	100 MHz to 1.1 THz
Material properties	Dielectric and magnetic
Sample form	Most often used for solid materials Sample is assumed to have flat parallel sides
Typical accuracy	1 to 2%
Data formats	Bi-static reflection (S21) in dB Data pane view displays trace data in tabular format
File formats	Data and Setup: .arc Data: .prn, .csv Measurement report: .pdf S-parameters: .s2p, .ts

Resonant cavity method – Option 003



Choose the resonant cavity method for thin films, substrate materials, and other low loss dielectric materials. The resonant cavity method uses a network analyzer to measure resonant frequency and Q of a resonant cavity fixture, first empty and then loaded with the sample under test. Permittivity can then be calculated from these measurements, knowing the volume of the sample, and some other parameters about the resonant cavity. Because it is a resonant method, only one frequency point is reported. However, it is much more sensitive and has better

resolution than the other techniques. Typical resolution for this method is 10^{-4} where the broadband method is 10^{-2} .

A least squares circle fitting technique is used to calculate Q, which uses both magnitude and phase information and is more repeatable than other Q calculation methods. The software then calculates ϵ_r' , ϵ_r'' and loss tangent and displays them in its easy to use interface.

Typical resonant cavity system configuration

- Keysight network analyzer

One or more resonant cavity fixtures:

- Split post dielectric resonators (SPDR) from QWED. These resonators are high quality and are available in frequencies from 1 GHz to 15 GHz. For more information, please email info@qwed.com.pl or visit <http://www.qwed.com.pl/hardware.html>
- ASTM D2520 standard waveguide resonators
- Keysight 85072A split cylinder resonator

A pair of test port cables

Adapters as required to connect cables to network analyzer and resonant cavity

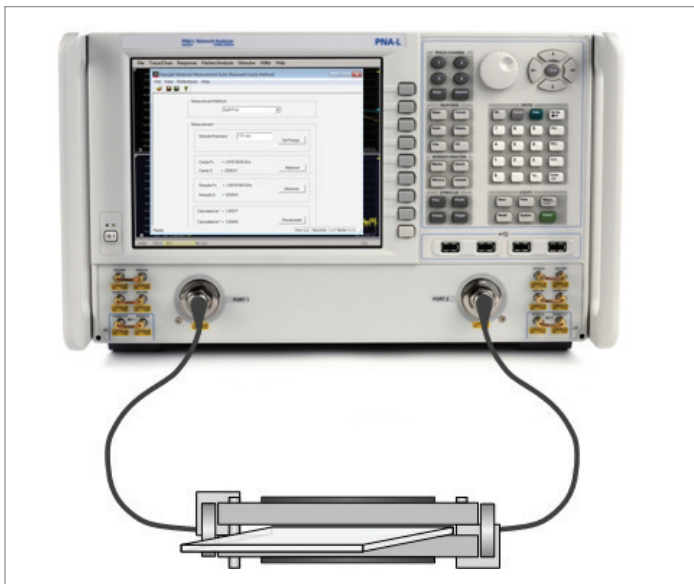


Figure 9. Resonant cavity system


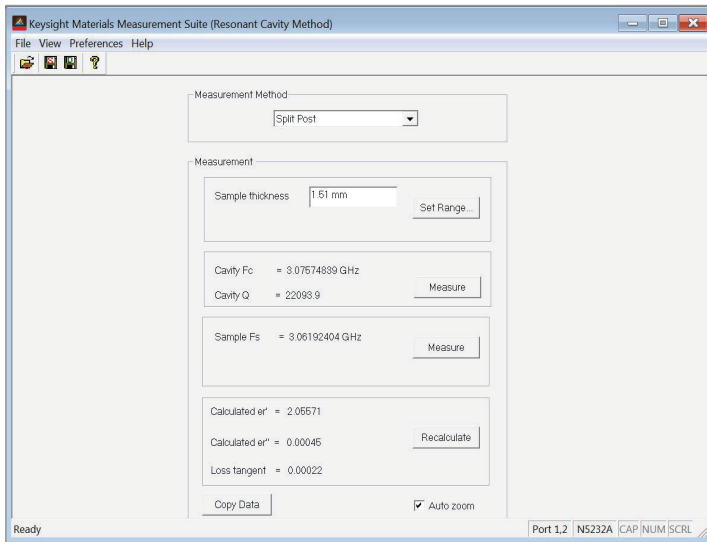


Figure 10. Resonant cavity method user interface

Typical frequency range	1 to 15 GHz
Material properties	Dielectric, low loss
Sample form	For split post and split cylinder resonator's, sample is thin sheet with flat parallel sides. For ASTM D2520 method, sample is a cylindrical rod shape.
Typical accuracy	1%, loss tangent resolution 1×10^{-4}
Data formats	Permittivity: ϵ_r' , ϵ_r'' , $\tan \delta$
File formats	Data and Setup: .cav Data: .prn

Coaxial probe method – Option 004



The coaxial probe method works with Keysight N1501A and 85070E series dielectric probe hardware. Measurements are conveniently made by immersing the probe into liquids or semi-solids – no special fixtures or containers are required. Measurements are non-destructive and can be made in real time. These important features allow the dielectric probe kit to be used in process analytic technologies.

Typical coaxial probe system configuration

- Keysight network analyzer
- Keysight N1501A or 85070E dielectric probe kit with cable and probe stand.
- Optional Keysight Ecal module for electronic calibration refresh. Electronic calibration refresh with ECal is not compatible with FieldFox network analyzers. ECal module requires USB connection to PC or PNA and ENA series network analyzers.
 - 8509xC Series
 - N469x Series
 - N443x Series (ports a and b only)

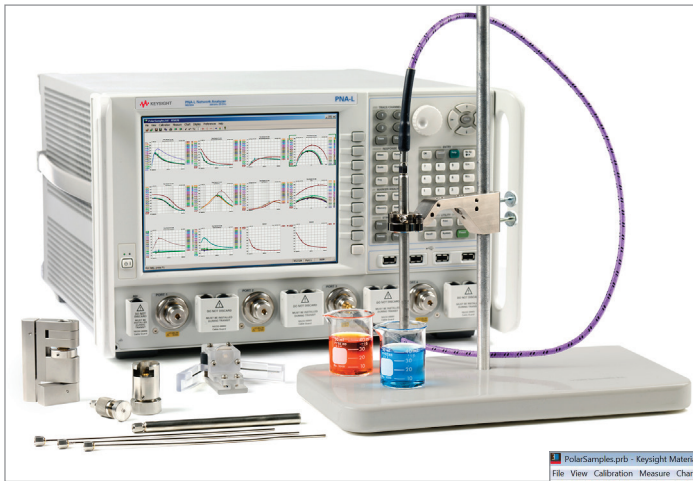


Figure 11. Coaxial probe system

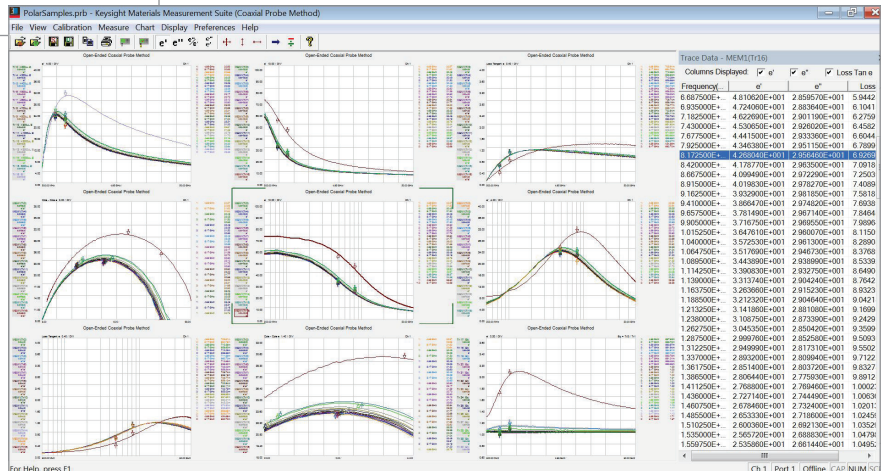


Figure 12. Example of coaxial probe measurement results

Calibration refresh reduces drift errors

The automated electronic calibration refresh feature recalibrates the system automatically, in seconds, just before each measurement is made. This virtually eliminates cable instability and system drift errors.

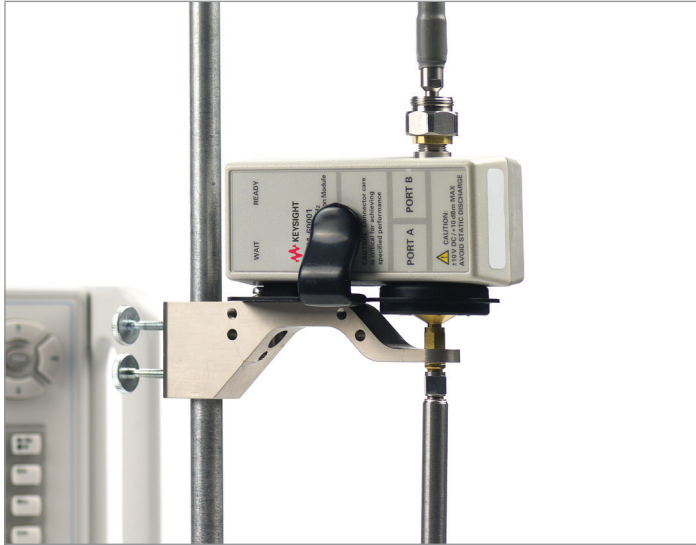


Figure 13. Ecal module connected in line for electronic

How it works:

A Keysight electronic calibration module (ECal) microwave ports are connected in line between the probe and the network analyzer test port cable. The ECal module USB communication port is connected either to the PC, PNA or ENA Series network analyzer running the N1500A software. The software guides you through a normal “three standard” calibration, (usually open, short, water), performed at the end of the probe. This calibration is then transferred to the ECal module. The ECal module remains in line and a complete ECal calibration is automatically performed before each measurement. Errors due to test port cable movement and system drift are removed by the new calibration.

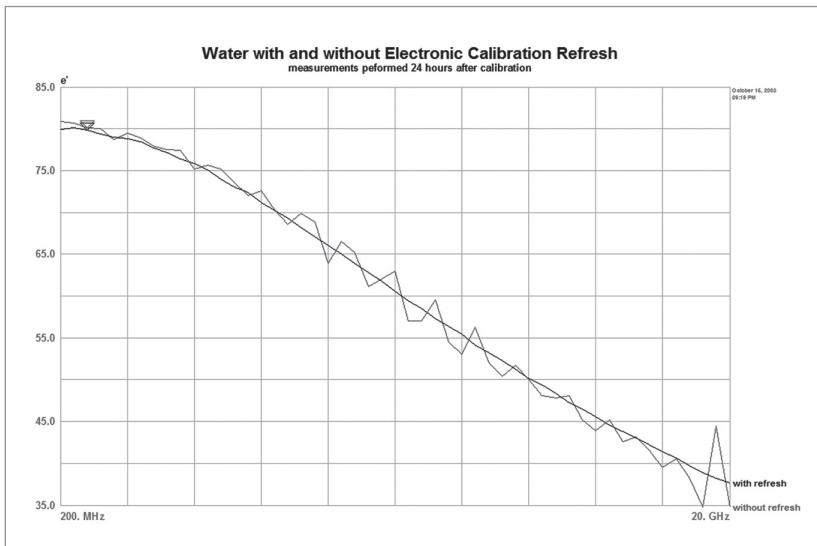


Figure 14. Water with and without electronic calibration refresh

This measurement shows the effects of system drift and cable instability on a dielectric measurement of water and the improvement with electronic calibration refresh. Both measurements were made 24 hours after the original calibration. The lighter colored, noisier, trace was made before the electronic calibration refresh was turned on. The darker, smoother, trace shows the improvement made after the electronic calibration refresh was turned on.

For systems without an ECal module, a simpler, “one standard” refresh calibration feature is also available, which can reduce the effects of system drift over time or temperature. After the initial “three standard” probe calibration is performed, the calibration can be refreshed at any time with the connection of a single standard. Any one of the three calibration standards can be defined as the refresh standard.

Multiple measurements utility

The multiple measurements utility automates multiple measurements over time. Enter the desired number of measurements and the time between the measurements and the utility will calculate the total time required. You can choose to have your measurements displayed or saved in .prn format data files. Click the Start Measurements button and let the software do the rest.

Figure 15. Multiple measurements utility

Suggested frequency range	200 MHz to 50 GHz with network analyzer 10 MHz to 3 GHz with E4991A impedance analyzer
Material properties	Dielectric only (non-magnetic)
Sample form	Best used for liquids or soft conformable solids
Typical accuracy	5-10%
Data formats	Permittivity: ϵ_r , ϵ_r , $\tan \delta$ S-parameters: log mag, linear mag, phase, unwrapped phase, group delay, smith chart, polar chart, real, imaginary, and SWR. Trace math functions: +, -, *, /, mean and standard deviation. Data pane view: displays trace data in tabular format.
File formats	Data and Setup: .prb, .tst Data: .prn, .csv Measurement report: .pdf S-parameters: .slp, .ts

Ordering information

N1500A Materials measurement suite

License includes 1 year software update service

N1500A-UL8 USB software security key – required for first time N1500A buyers to run software suite. One key works with multiple method options.

Choose one or more method options:

- N1500A-001 Transmission line and free space method
- N1500A-002 Arch reflectivity method
- N1500A-003 Resonant cavity method
- N1500A-004 Coaxial probe method

Required, but not included:

- Compatible network analyzer – for a complete up to date list of supported analyzers, please see <http://na.support.keysight.com/materials/docs/N1500A-VNAs.pdf>
- PC (optional with ENA and PNA series network analyzers when software is installed directly on analyzer).
 - Windows XP, Windows 7 or Windows 8 Operating System
 - Keysight IO Libraries Suite version 16.1 or later
 - GPIB, LAN or USB interface depending on network analyzer. For network analyzer interface information, please see <http://na.support.keysight.com/materials/docs/N1500A-VNAs.pdf>
- Internet access for license redemption
- Appropriate fixtures and cables for chosen measurement method. Please see method option descriptions in this document for more information.

N1500AU Materials measurement suite -- 1 year software update service (SUS)

Choose one or more method options:

- N1500AU-010 Transmission line and free space method SUS
- N1500AU-020 Arch reflectivity method SUS
- N1500AU-030 Resonant cavity method SUS
- N1500AU-040 Coaxial probe method SUS

Upgrade Information



Customers who own 85070E or 85071E licenses can upgrade to N1500A by purchasing the N1500AU materials measurement suite software update service and desired options. Licenses will be tied to the 85070E or 85071E USB software security key.

Customers who own the 8507xA/B/C/D version software must purchase N1500A with appropriate method option and USB software security key.

To Upgrade From	Order
85070E	N1500AU-004
85071E	N1500AU-001
85071E-100	N1500AU-001
85071E-200	N1500AU-002
85071E-300	N1500AU-003
85070A/B/C/D	N1500A-004 N1500A-UL8
85071A/B/C/D	N1500A-001 N1500A-UL8

From Hewlett-Packard through Agilent to Keysight

For more than 75 years, we've been helping you unlock measurement insights. Our unique combination of hardware, software and people can help you reach your next breakthrough. **Unlocking measurement insights since 1939.**



For more information on Keysight Technologies' products, applications or services, please contact your local Keysight office. The complete list is available at: www.keysight.com/find/contactus

Americas

Canada	(877) 894 4414
Brazil	55 11 3351 7010
Mexico	001 800 254 2440
United States	(800) 829 4444

Asia Pacific

Australia	1 800 629 485
China	800 810 0189
Hong Kong	800 938 693
India	1 800 11 2626
Japan	0120 (421) 345
Korea	080 769 0800
Malaysia	1 800 888 848
Singapore	1 800 375 8100
Taiwan	0800 047 866
Other AP Countries	(65) 6375 8100

Europe & Middle East

Austria	0800 001122
Belgium	0800 58580
Finland	0800 523252
France	0805 980333
Germany	0800 6270999
Ireland	1800 832700
Israel	1 809 343051
Italy	800 599100
Luxembourg	+32 800 58580
Netherlands	0800 0233200
Russia	8800 5009286
Spain	800 000154
Sweden	0200 882255
Switzerland	0800 805353
	Opt. 1 (DE)
	Opt. 2 (FR)
	Opt. 3 (IT)
United Kingdom	0800 0260637

For other unlisted countries:
www.keysight.com/find/contactus
 (BP-02-10-16)



www.keysight.com/go/quality
 Keysight Technologies, Inc.
 DEKRA Certified ISO 9001:2015
 Quality Management System

This information is subject to change without notice.
 © Keysight Technologies, 2014-2016
 Published in USA, March 24, 2016
 5992-0263EN
www.keysight.com

myKeysight

myKeysight

www.keysight.com/find/mykeysight

A personalized view into the information most relevant to you.



Three-Year Warranty

www.keysight.com/find/ThreeYearWarranty

Keysight's committed to superior product quality and lower total cost of ownership. Keysight is the only test and measurement company with three-year warranty standard on all instruments, worldwide. And, we provide a one-year warranty on many accessories, calibration devices, systems and custom products.



Keysight Assurance Plans

www.keysight.com/find/AssurancePlans

Up to ten years of protection and no budgetary surprises to ensure your instruments are operating to specification, so you can rely on accurate measurements.

Keysight Infoline

www.keysight.com/find/service

Keysight Infoline

Keysight's insight to best in class information management. Free access to your Keysight equipment company reports and e-library.

Keysight Channel Partners

www.keysight.com/find/channelpartners

Get the best of both worlds: Keysight's measurement expertise and product breadth, combined with channel partner convenience.

www.keysight.com/find/materials